



Figure 1 Weight Increase of the Three Pads

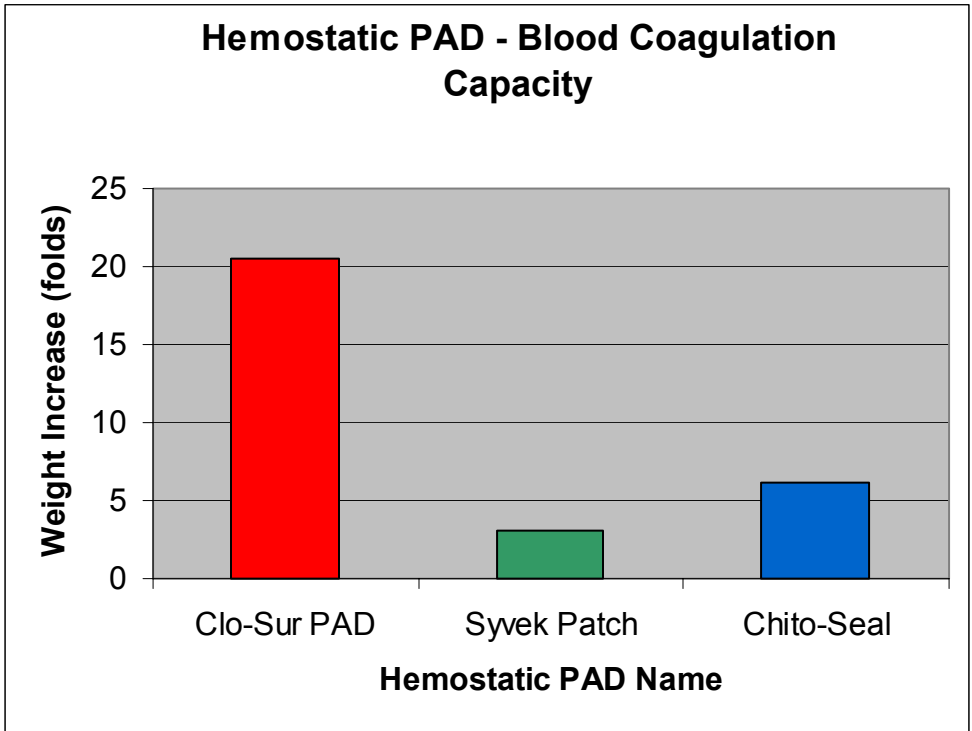

Notes 1: Hemostatic Pad's Blood Coagulation capacity is determined by the Pad's ability to increase its own weight by absorbing and/or coagulating surrounding blood

Figure 2 Normalized Weight Increase of the Three Pads

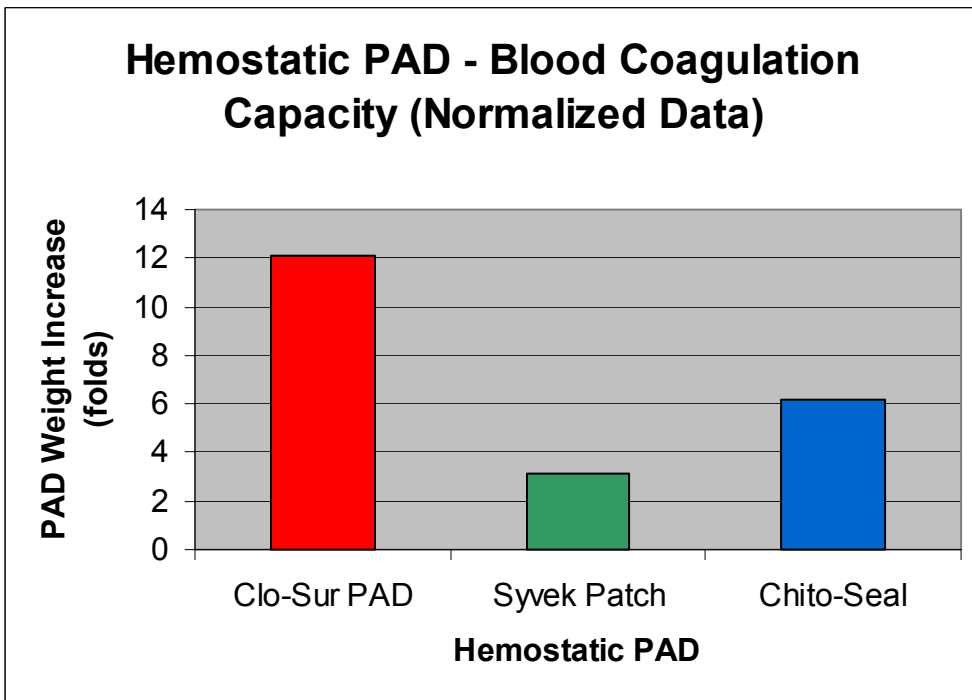

Note 1: Normalized data factors-in the weight of each manufacturers Pad to make results equivalent for all Pads tested.